

this document brought to you by
AED Superstore

ZOLL AED 3 Trainer Operator's Guide

Learn how to set-up, use, and maintain your ZOLL AED 3
Trainer.

800.544.0048
AEDSuperstore.com

ZOLL AED 3[®]

TRAINER



Operator’s Guide



ZOLL Medical Corporation
269 Mill Road
Chelmsford, MA USA
01824-4105

Attn: Technical Service Department

Tel: 978-421-9655 800-348-9011
Fax: 978-421-0001



ZOLL International Holding B.V.
Newtonweg 18
6662 PV ELST
The Netherlands

Tel: +31 (0) 481 366410
Fax: +31 (0) 481 366411

International Service: Contact your local distributor.

The ZOLL AED 3® Trainer is used to demonstrate and practice complete Sudden Cardiac Arrest rescue simulations, including delivering shocks and performing CPR.

The following items are included in the shipping box:

- Qty 1: ZOLL AED 3 Trainer
- Qty 1: ZOLL AED 3 Trainer CPR Uni-padz® Electrode Training Harness, Electrode Pads, and Liners
- Qty 4: D-cell Batteries
- Qty 1: ZOLL AED 3 Trainer Operator’s Guide

Features of the ZOLL AED 3 Trainer

- Integrated Real CPR Help®: The ZOLL AED 3 Trainer incorporates real-time compression feedback (rate and depth) during compressions when using the ZOLL AED 3 Trainer CPR Uni-padz.
- “Pads On” manikin detection: The ZOLL AED 3 Trainer moves to the “analysis” state once the trainee places the CPR Uni-padz on the manikin.
- Active LCD Display: The full color display mimics the ZOLL AED 3 and displays rescue images along with the real-time compression bar when the trainee is performing compressions.
- Easy Configuration: Configuration is performed directly on the trainer. There is no need for a remote control. Available options include:
 - Training scenario
 - Operating mode (SEMI-AUTOMATIC or FULLY AUTOMATIC)
 - Lay Rescuer Prompts (ON/OFF)
 - Check Breathing Prompts (ON/OFF)
 - Real CPR Help Prompts (ON/OFF)
 - Volume
 - Language (select models only)
- Adult/Child Operation
- Semi-Automatic/Fully Automatic: One trainer for both types of devices. The ZOLL AED 3 Trainer can easily convert from a Semi-Automatic mode to a Fully Automatic mode.
- Long lasting training pad: The electrode pads are designed to last for a minimum of 50 training cycles. The electrode harness is designed to last for a minimum of 100 training cycles. A training cycle is defined as two minutes of manikin compressions, performed at a depth of 2” and a rate of 100 per minute. Each cycle also includes one pad-to-manikin application and removal, and one

pad-to-liner application and removal. Sternum and Apex pads should remain adhered to the manikin.

- USB Software Updates: The trainer’s software is easily updated using a USB flash drive with preloaded software.
 - **NOTE:** Leaving a USB flash drive installed in the USB Connector during training will reduce the battery life and impact the performance of the ZOLL AED 3 Trainer.

Proper Use and Care of Electrode Pads

- Before use, remove the electrode pads from the plastic liners by grasping each pad at the black arrow and carefully peeling away from its liner at a 90° angle.
- When not in use during the training session, place the electrode pads back on the plastic liners and store in the plastic bag in the rear pocket of the ZOLL AED 3 Trainer.
- The adhesive gel surface of the electrode pads should be applied only to the clean and dry surface of the plastic liner, or directly to the dry skin surface of a CPR training manikin that has been appropriately cleaned of any residual oils, dirt or debris.
- When training is complete, carefully remove the electrode pads from the CPR training manikin by grasping the pads at the black arrow and carefully peeling away from the manikin at a 90° angle.
- Carefully reapply the electrode pads to the plastic liners ensuring each pad is completely flat and fully adhered to its liner.

ZOLL AED 3 Trainer

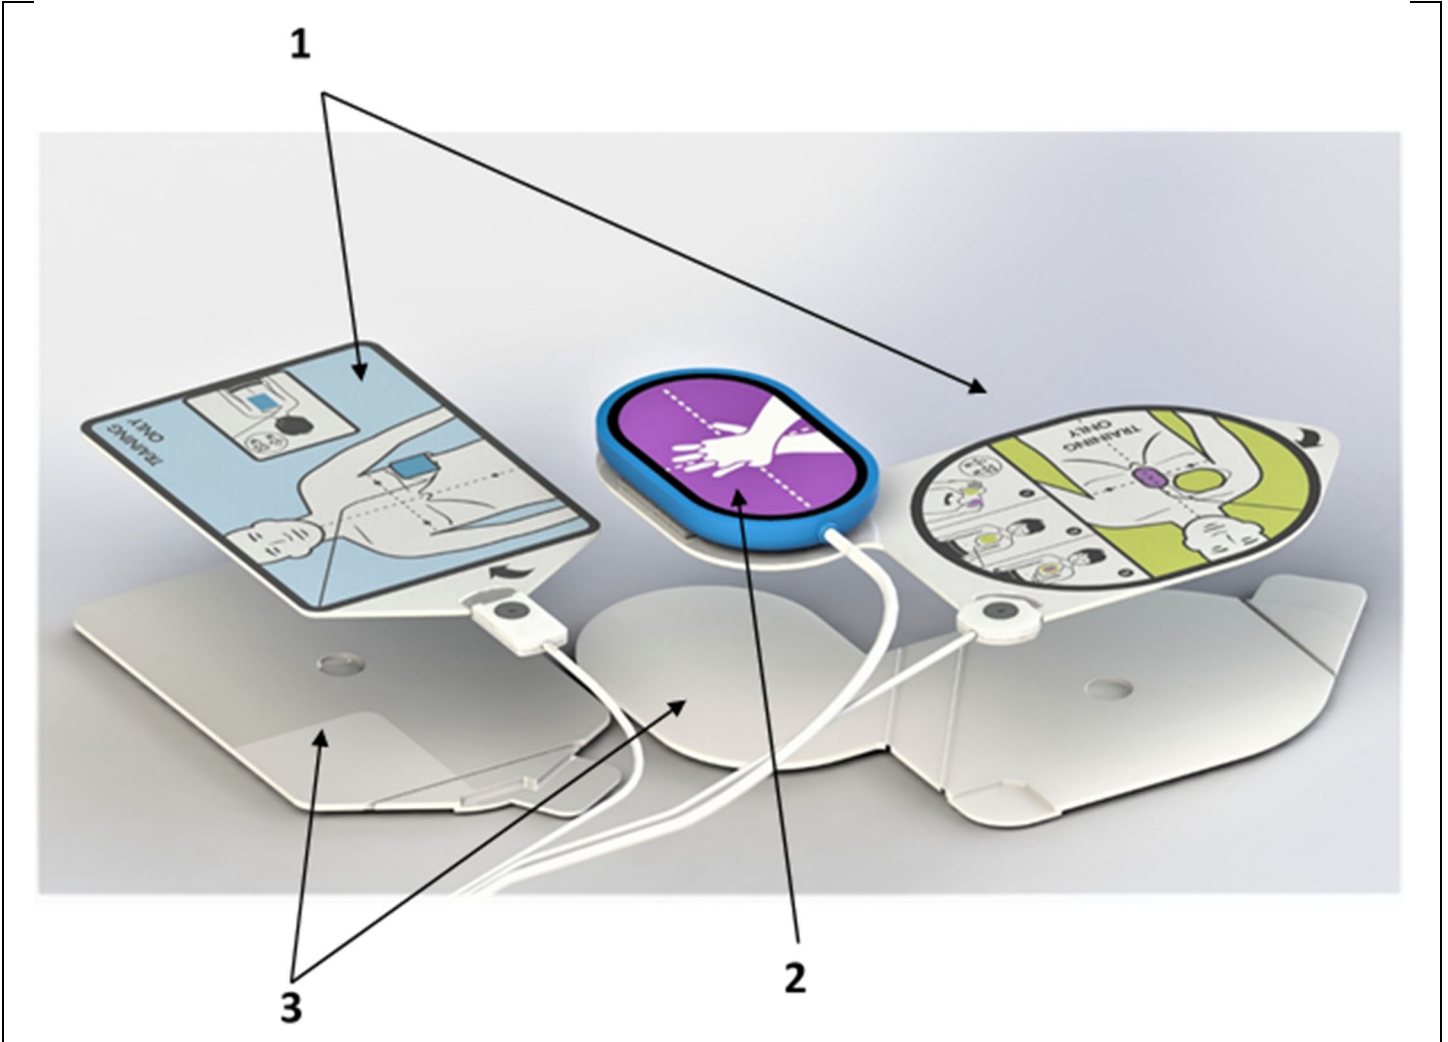
 <p>The image shows the front of the ZOLL AED 3 Trainer. It is a green and blue device with a central screen. Callout 1 points to a power button on the left. Callout 2 points to a green checkmark indicator at the top. Callout 3 points to a blue connector on the right side. Callout 4 points to a lightning bolt shock button below the screen. Callout 5 points to a child button with a person icon on the right. Callout 6 points to a speaker grille on the bottom left.</p>	<p>Front of ZOLL AED 3 Trainer</p> <ul style="list-style-type: none">1 – ON/OFF Button2 – Replicated Status Indicator3 – Training Electrode Connector4 – Shock Button5 – Child Button6 - Speaker
 <p>The image shows the rear of the ZOLL AED 3 Trainer. Callout 1 points to a USB connector on the left. Callout 2 points to a label at the top with technical specifications. Callout 3 points to a serial number label below it. Callout 4 points to the battery compartment door in the center. Callout 5 points to a kick-stand at the bottom.</p>	<p>Rear of ZOLL AED 3 Trainer</p> <ul style="list-style-type: none">1 – USB Connector2 – Device Identification Label3 – Device Serial Number Label4 – Battery Compartment Door5 – Support Kick-stand

ZOLL AED 3 Trainer Operational Buttons



- 1 – Training Scenario Pause Button
- 2 – Device Configuration Menu Selection Button
- 3 – Device Configuration Menu Scroll Button
- 4 – Device Configuration Option Selection Button


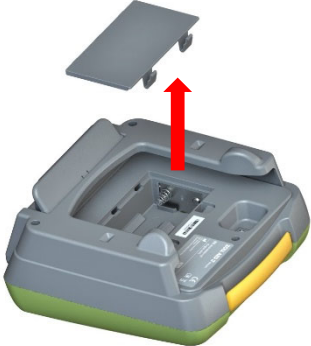


ZOLL AED 3 Trainer CPR Uni-padz Training Electrodes



- 1 – ZOLL AED 3 Trainer CPR Uni-padz Electrode Pads
- 2 – ZOLL AED 3 Trainer CPR Uni-padz Electrode Training Harness
- 3 – ZOLL AED 3 Trainer CPR Uni-padz Electrode Liners

When you receive your ZOLL AED 3 Trainer the training electrodes will need to be assembled. Please refer to the ZOLL AED 3 Trainer Electrode Attachment Guide (P/N 9650-000864-40) for assembly instructions.

Setting up your ZOLL AED 3 Trainer

Installing Batteries	
(1)	
(2)	
(3)	
(4)	

Insert CPR Uni-padz Electrodes into Training Electrode Connector

(1)



(2)



(3)



Configuring the ZOLL AED 3 Trainer

Enter the Setup/Configuration menu by pressing the Device Configuration Menu Selection Button.

Navigation Instructions:

- (1) Use the “Device Configuration Menu Scroll Button” button to progress from option to option.
- (2) Use the “Device Configuration Option Selection Button” button to adjust a configuration option.
- (3) When setup is complete press the “Device Configuration Menu Selection Button” to turn the trainer off.

Configurable options:

- (1) Select your Training Scenario from the four options (⚡=Shock Icon, ⚡=No Shock Icon)

a. Shock / Shock / Shock	⚡ / ⚡ / ⚡
b. No Shock / Shock / Shock	⚡ / ⚡ / ⚡
c. Shock / No Shock / No Shock	⚡ / ⚡ / ⚡
d. No Shock / No Shock / No Shock	⚡ / ⚡ / ⚡

- (2) Device Operation / Shock Type:
 - a. SEMI-AUTOMATIC
 - b. FULLY AUTOMATIC
- (3) Lay Rescuer Prompts (“CHECK RESPONSIVENESS” / “CALL FOR HELP”)
 - a. ON
 - b. OFF
- (4) Check Breathing Prompts (“OPEN AIRWAY” / “CHECK BREATHING”):
 - a. ON
 - b. OFF
- (5) Real CPR Help Prompts (“PUSH HARDER” / “GOOD COMPRESSIONS”):
 - a. ON
 - b. OFF
- (6) Volume (Low, Medium, High -- indicated by Icon):
 - a. ■■■ - Low
 - b. ■■■ - Medium
 - c. ■■■ - High
- (7) Language (specified by model)

Troubleshooting

Real CPR Help prompts and Software Updates will not function in low battery conditions. The prompt “CHANGE BATTERY” will be displayed in the setup menu when the battery is low.

Maintenance

The ZOLL AED 3 Trainer should be kept clean, undamaged, and free of excessive wear.

Verify that there are no cracks or loose parts in ZOLL AED 3 Trainer.

The ZOLL AED 3 Trainer CPR Uni-padz Electrode Training Harness should be replaced as necessary.

The ZOLL AED 3 Trainer CPR Uni-padz Electrode Pads should be replaced as necessary.

The ZOLL AED 3 Trainer CPR Uni-padz Electrodes Liners should be replaced as necessary.

Cleaning

The ZOLL AED 3 Trainer may be cleaned with a soft, damp cloth using soap and water, then wiped dry immediately.

DO NOT:

- Immerse any part of the trainer in water.
- Use ketones (e.g., MEK, acetone) to clean the trainer
- Use abrasives on any surface.
- Sterilize the ZOLL AED 3 Trainer.

Accessories

The following ZOLL AED 3 Trainer accessories may be ordered from the ZOLL Customer Service Department or your local distributor:

8028-000010: ZOLL AED 3 Trainer CPR Uni-padz Electrode Training Harness

8028-000014: ZOLL AED 3 Trainer CPR Uni-padz Electrode Pads, Qty 5

8028-000013: ZOLL AED 3 Trainer CPR Uni-padz Electrode Replacement Liners, Qty 1

Warnings

The ZOLL AED 3 Trainer is intended for indoor use only.

The ZOLL AED 3 Trainer is intended for training purposes only. It will not deliver defibrillation energy.







Do not attempt to plug the AED Simulator into the connector of ZOLL AED 3 Trainer.

Do not attempt to take the ZOLL AED 3 Trainer apart.

Remove battery compartment doors only to replace batteries.

Symbols

Any or all of the following symbols may be used in this manual or on this device:

	Conformité Européenne - Complies with Low Voltage Directive 73/23/EEC.
	Consult instructions for use.
	Return to a collection site intended for waste electrical and electronic equipment (WEEE). Do not dispose of in unsorted trash.
	Catalogue Number.
	Manufacturer.
	Authorized representative in the European Community.